


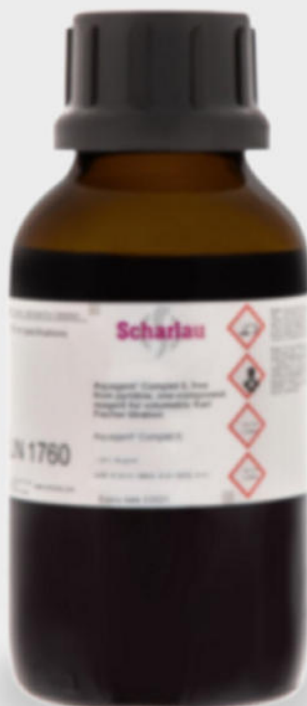

Application Note AN-K-073

Volumetric Karl Fischer titration with Scharlau Aquagent® reagents

Test measurements using Aquagent® Complet 5 and Methanol Fast

This Application Note summarizes a series of test measurements performed with an OMNIS KF Titrator and Karl Fischer reagents Aquagent® Complet 5 and Methanol Fast from Scharlau.

Three series of titer determinations using various water standards were carried out. The results obtained using different water standards were found

to lie in a similar range. The reproducibility of the results was determined to be very good.

Using an OMNIS titration system from Metrohm and the Scharlau Karl Fischer reagents, titer determinations can be carried out quickly without any decline in the reproducibility of results.

STANDARDS

Three different water standards have been used for the tests performed in this study:

1. Water standard with a water content of approximately 10.0 mg/g («water standard 10»)
2. Sodium tartrate dihydrate with a water content of approximately 15.7%
3. Deionized water

EXPERIMENTAL

A 10-fold titer determination was carried out with both water standards and the deionized water.

The sample sizes were varied for water standard 10 (between 0.5 g and 4.0 g) as well as for the sodium tartrate dihydrate (between 0.077 g and 0.114 g). A constant sample size of 25 µg was used for the

deionized water.

The water standard 10 was added with a glass syringe. To add the sodium tartrate dihydrate, a weighing boat (6.2412.000) was used. The deionized water was injected into the titration cell with a microliter syringe.

RESULTS

The following table shows the results of three titer determination series using using Aquagent® Complet

5 and Methanol Fast reagents from Scharlau.

Table 1. Results of the titer determination series (n = 10) with three water standards.

Standard	Titer in mg/mL	s(abs) in mg/mL	s(rel) in %
1	5.3936	0.02248	0.09
2	5.3781	0.00485	0.16
3	5.3459	0.00873	0.42

The titer determinations were both fast and reproducible. The relative standard deviations were very low, especially for the water standard 10 and the sodium tartrate dihydrate.

Methanol Fast contains additives to accelerate the titration, therefore it is recommended to use the method parameters suitable for two-component reagents (**Table 2**).

Table 2. List of suitable method parameters for two-component reagents in OMNIS.

Parameter	Value
Dynamics	300 mV
Max. rate	max
Min. volume increment	min
I _{pol}	50 µA
EP	250 mV

CONTACT

Metrohm France
13, avenue du Québec - CS
90038
91978 VILLEBON
COURTABOEUF CEDEX

info@metrohm.fr

CONFIGURATION



OMNIS Titrator KF

L'OMNIS Titrator KF vous offre un ensemble complet pour le titrage volumétrique Karl Fischer. L'ensemble contient un OMNIS Basic Titrator avec agitateur magnétique pour le titrage potentiométrique à point final prédéfini, la licence fonctionnelle KFT avec conditionnement, l'OMNIS Solvent Module et les accessoires au complet pour le titrage volumétrique Karl Fischer.

Tirez donc profit de l'extraordinaire facilité d'utilisation, avec démarrage du titrage automatique après ajout d'échantillon et sécurité maximale grâce à une manipulation des réactifs sans contact à l'aide du 3S-Liquid Adapter et de l'OMNIS Solvent Module.