



Application Note AN-NIR-086

ディーゼル排気液 (DEF) の品質管理

Fast determination of urea content with high accuracy

(DEF) (ISO 22241-2:2019) (HPLC)DS2500(DEF)-

(Vis-NIR) (DEF)1

DS2500(DEF)-(Vis-NIR)(DEF)1




1.


1.

DS2500 Liquid Analyzer	2.929.0010
Disposable vials, 2 mm diameter, transmission	6.7492.000
Vision Air 2.0 Complete	6.6072.208

16Vis-NIR (2)NIR(FOM)()

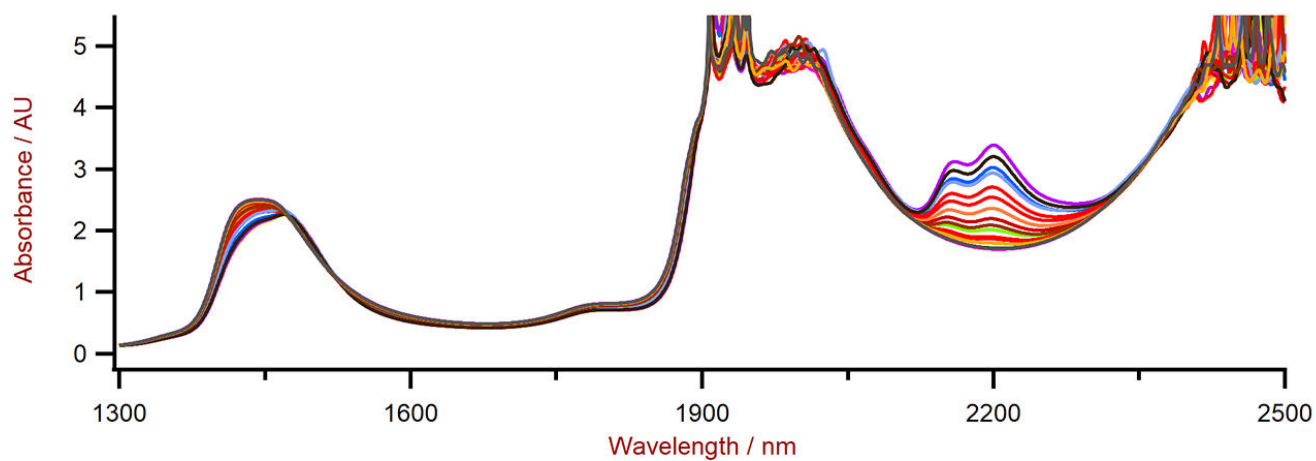

2. DS2500DEFVis-NIR

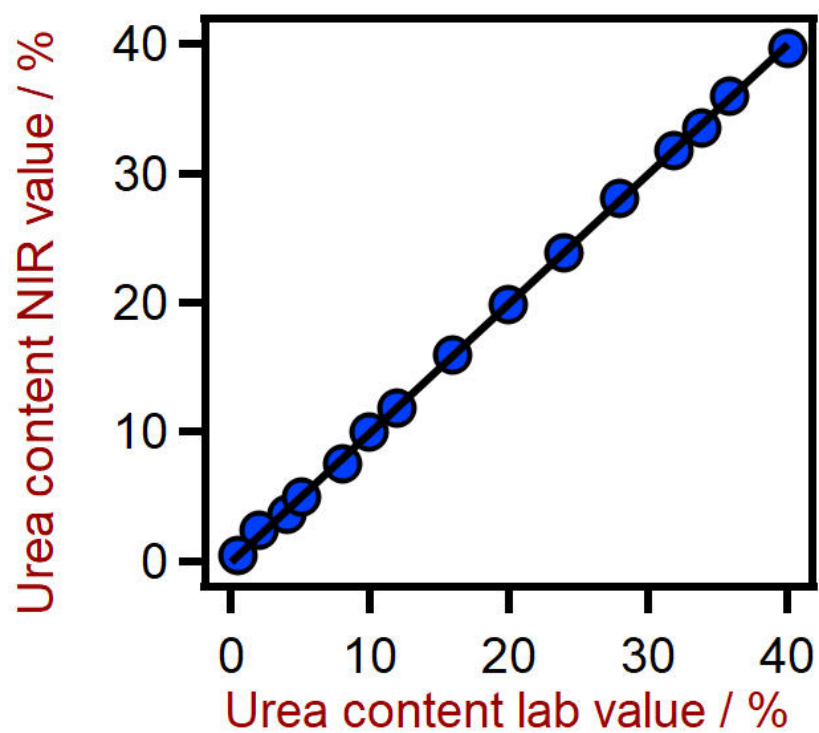

3. DS2500

2:DS2500(FOM)

R_2	0.999
(SEC)	0.23%
(SECV)	0.25%

(DEF)DS2500Vis-NIR()NIR

3.HPLC

HPLC	5 () + 10 (HPLC)

Internal reference: AW NIR CH-0015-051520

CONTACT

143-0006 6-1-1
null 9

metrohm.jp@metrohm.jp



DS2500 Liquid Analyzer

NIRS DS2500 Liquid Analyzer
NIRS DS2500 Liquid Analyzer

DS2500 Liquid Analyzer 400~2500 nm80°CDS2500
Liquid Analyzer1Vision Air

Metrohm



2mmDS2500

2 mm



Vision Air 2.0 Complete

Vision Air -

Vision Air Complete

Vision Air :

-
-
- SQL

Vision Air Complete (66072208) :

-
-
-

Vision Air Complete :

- 66072207 (Vision Air Network Complete)
- 66072209 (Vision Air Pharma Complete)
- 66072210 (Vision Air Pharma Network Complete)