


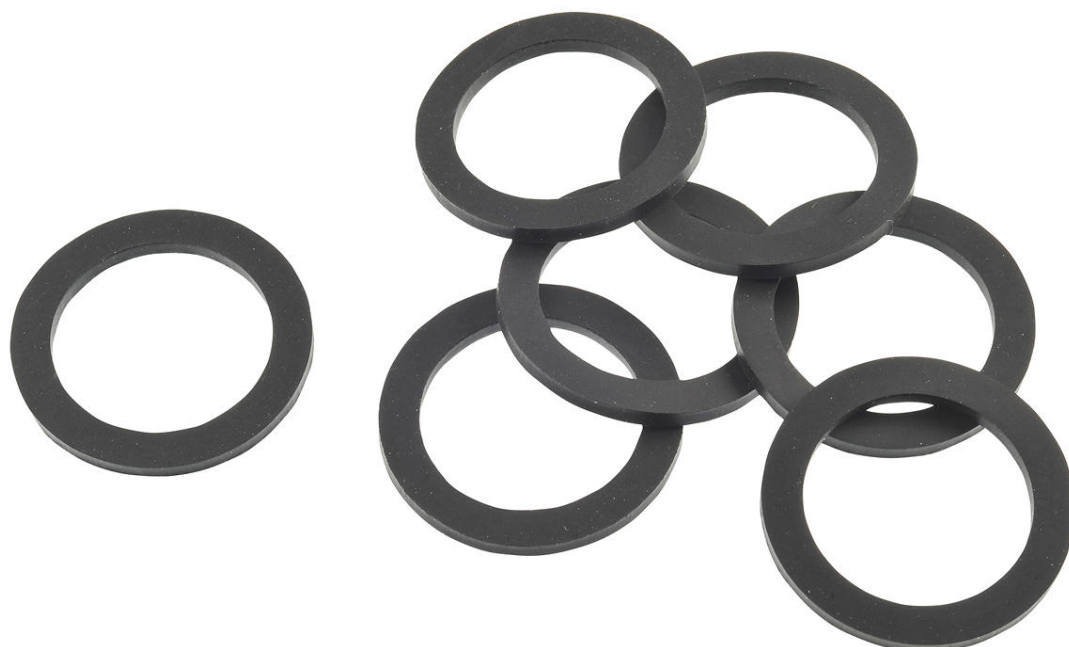

KF Dis-Cover6.02710.010

6.05700.170

6.02710.01016

Order no.

6.02710.010 **KF Dis-Cover lid for OMNIS 120 mL sample beaker, 16 pieces**

Lid with seals for volumetric Karl Fischer Titration in 6.01400.200, 6.01400.300 and 6.01400.303 sample beakers in the OMNIS Sample Robot Pick&Place system.

